

Dual Tree M-Band Wavelet Transform Model based Classification of Mammogram Images

Dr. C.SUBA and Dr. S.Niranjana,

Asst. Professor in Computer Science, Sri Lakshmi College of Arts & Science, Bangoram, India
HOD & Associate Professor in BCA, Mohamed Sathak College of Arts & Science, Sholinaganalur, Chennai. India

Abstract

Breast Cancer is the one of the leading causes of cancer mortality among women and second leading cause of cancer deaths worldwide after lung cancer. In the US, 1 in 8 women will be diagnosed with breast cancer in their lifetime. The risk for breast cancer increases with age; most breast cancer are diagnosed after age 50 and about 95% of all breast cancers in the US occur in women 40 and older.

Keywords:

MIAS images, Dual Tree M-Band Wavelet Transform and Support Vector Machine

accuracy of 98.19%, sensitivity of 97.09% and specificity of 99.35%. Muhammad Talha used Programming (GP) based filter is proposed, while the fusion of Discrete Cosine Transform (DCT) and Discrete Wavelet Transform (DWT) features is used as an input to classifier. It achieve 96.97% accuracy, 98.39% sensitivity and 94.59% specificity for classifying mammograms into normal and abnormal (cancer) categories using SVM (Support Vector Machine) classifier and MIAS (Mammographic Institute Society Analysis) dataset.

1. Introduction

Breast cancer is disease that is diagnosed among the women in the world [1, 2]. Mammography is used as early screening tool for breast cancer & Mammographic images are X-ray images of breast region [3]. To objective of this paper is to build a Computer Aided Diagnosis (CADx) model for performance of mammogram classification system using variance features is discussed. To classifying mammogram images into three stages; normal/abnormal in stage 1, Microcalcifications (MCs)/Mass in stage 2, benign/malignant in stage 3.

2. Related Work

Various kinds of techniques have been proposed to improve the accuracy of breast cancer classification. The research in the areas of CAD systems for breast cancer detection and classification has been conducted in last few decades. R. Nithya and B. Santhi [4] using GLCM (Grey Level Co-occurrence Matrix) features. The highest classification accuracy obtained by this approach was 96% on mammograms from the DDSM. Aidarus M. Ibrahim, Baharum Baharudin, Abas Md Said and P.N. Hashimah et al. [5] proposed k-means clustering coupled with max pooling (k-means-max pooling) is compared with well known feature extraction method namely Bag-of-features combined two different classifier; K-Nearest Neighbor (KNN) and Support Vector Machine (SVM), achieved good performance with an average classification

3. Methodology

An overview of proposed method is presented in Figure 1.

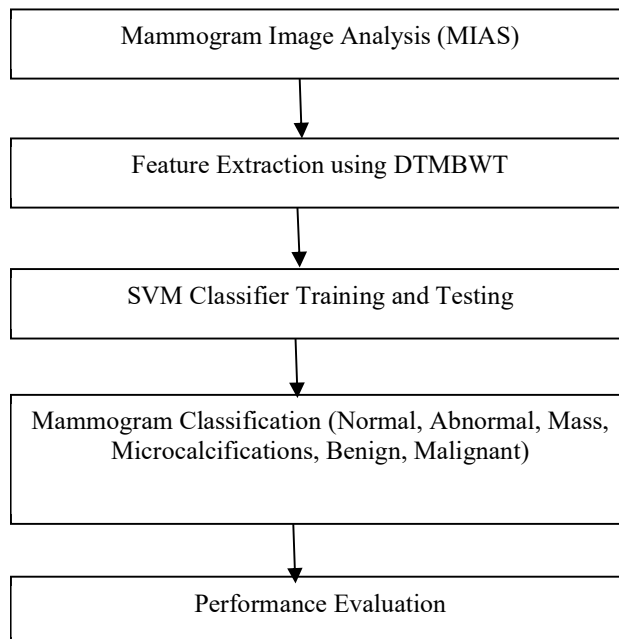


Figure 1: An Overview of Proposed Method

3.1 Data Collection

The most popular easily accessed databases and therefore the most commonly used databases are the Mammographic Image Analysis Society (MIAS) database and the Digital Database for Screening Mammography (DDSM). The Mammographic Image Analysis Society (MIAS) is an organization of UK research groups interested in the understanding of mammograms and has generated a database of digital mammograms. The database contains 322 digitized films and is available on 2.3 GB [6].

3.2 Feature Extraction

Feature extraction is very important part of pattern classification. In pattern recognition, feature extraction is considered as a critical process; owing to the features obtained from this process the efficacy of the classification process is directly influenced. Hence, feature with rich discriminative nature will assist the classification system effectively while the lack of such discriminative nature can slow down the classification process from accurate identification. Feature extraction using DTMBWT is performed by the following three computational modules. 1) ROI Selection 2) DTMBWT 3) Feature Computation [7, 8].

3.3 Classification

This is the final stage of the proposed mammogram classification system where the unknown mammogram is labelled into one of the predefined category of mammogram i.e. normal/abnormal, mass/MCs and abnormal severity into benign/malignant. A sequential classification stage that consists of three stages is designed for the classification of the given mammogram image using supervised learning based SVM classifier. In each stage, the performance of SVM classifier is analysed using five kernel functions; linear, quadratic, polynomial, Radial Basis Function (RBF) and Multilayer Perception (MLP).

4. Performance Measure

The performance of the prediction was evaluated in terms of classification accuracy, sensitivity, specificity, confusion matrix with Receiver Operating Characteristic (ROC) curve.

4.1 Classification Accuracy

The classifier performance is better if it has higher classification accuracy. It is defined by

$$\text{Classification rate (\%)} = \frac{\text{Total number of correctly classified images}}{\text{Total number of images}} \times 100$$

4.2 Sensitivity

The sensitivity measure was first introduced in medical domain to ensure the test ability of the classifier [9]. It is calculated in the same way as the classification accuracy sensitivity was computed as a number of true positive decisions over a number of actual positive cases. It can be represented as follows:

$$\text{Sensitivity } y = \frac{TP}{(TP + FN)}$$

where TP = True Positive cases and FN = False Negative cases.

4.3 Specificity

The specificity measure was also established in medical domain and computed in the same fashion as sensitivity [10]. The specificity can be calculated as the number of true negative decisions over the number of actual negative cases. It can be represented as follows:

$$\text{Specificity } y = \frac{TN}{(FP + TN)}$$

4.4 Confusion Matrix

For a two class problem, confusion matrix is constructed by using the classifier outcome with the actual one. Table 1 shows the confusion matrix.

Table 1 Confusion Matrix

Test outcome	Actual Class	
	Class 1	Class 2
Class 1	True Positive	False Positive
Class 2	False Negative	True Negative

In Table 1

- ✓ **True positive** : class 1 object is correctly classified as class 1 object
- ✓ **False Positive** : class 2 object is incorrectly classified as class 1 object
- ✓ **True Negative** : class 2 object is correctly classified as class 2 object
- ✓ **False Negative** : class 1 object is incorrectly classified as class 2 object

4.5 ROC Curve

ROC curve is very useful for visualizing and analysing the performance of a classifier. It shows the tradeoff between benefits (TP) and costs (FP). In addition, Area under the Curve (AUC) indicates the classifier performance.

5. Experiment Result

This section deals with experimental results of the evaluated mammogram classification system and their implications are discussed.

5.1 First Stage Classification System

The evaluated results of first stage classification system using variance features are illustrated in this section. Table 1 shows the classification accuracy of first stage classification.


Table 2: Classification Accuracy for Normal/Abnormal Classification System (1st stage) based on DTMBWT Variance Features and SVM Classifier

Level	Overall Classification Accuracy		
	Benign	Malignant	Average
Polynomial			
1	96.74	49.29	73.01
2	94.10	50.45	72.28
3	90.92	54.93	72.92
4	86.02	80.98	83.50
5	78.29	73.82	76.05
6	67.86	73.58	70.72


The interpretations of Table 2 are as follows:

The maximum average classification accuracy while utilizing variance feature is 83.50%. Among the five kernels used for normal and abnormal image classification, polynomial kernel achieves maximum classification accuracy while using 4th level variance features of DTMBWT. Maximum average classification accuracy by linear, quadratic, RBF and MLP kernel is 75.76%, 72.30%, 74.55%, 70.00% respectively. It is also observed that all SVM kernels produce over 70% accuracy while using variance features.

In order to visualize the performance of the proposed 1st stage classification using DTMBWT variance features and SVM classifier, confusion matrices and ROC plot are shown in Figure 2.

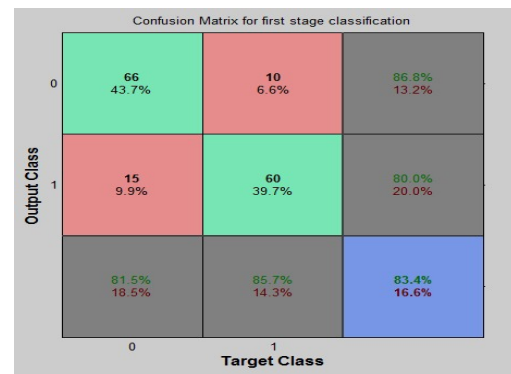

(a) Confusion matrix

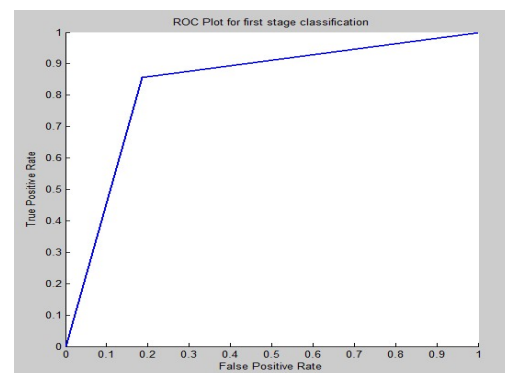

(b) ROC plot

Figure 2: Performance of 1st Stage Classification using DTMBWT Variance Features with Polynomial Kernel

It is observed from the Figure 2 that the 0.834 AUC is achieved while using Polynomial Kernel. It is observed from the Figure 2 that the sensitivity of the proposed system is 81.5% with a specificity of 85.7%. Figure 3 shows overall analysis of classification analysis of evaluated system in stage 1.

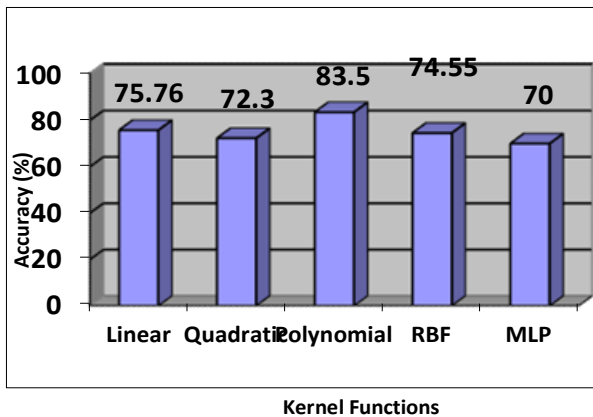


Figure: 3 Classification Accuracy vs. SVM Kernels for 1st Stage Classification using DTMBWT Variance Features

5.2 Second Stage Classification System

The evaluated results of 2nd stage classification system using variance features to classify the type of abnormality into mass or MCs are illustrated in this section. Table 3 shows the Classification Accuracy of 2nd Stage Classification.


Table 3 Classification Accuracy for Mass/MCs Classification System (2nd stage) based on DTMBWT Variance Features and SVM Classifier

Level	Overall Classification Accuracy		
	Benign	Malignant	Average
Linear Kernel			
1	89.40	33.29	61.35
2	85.04	45.30	65.17
3	58.07	61.31	59.69
4	81.12	79.99	80.56
5	74.92	63.49	69.20
6	62.70	62.97	62.83


Interpretations of Table 3 are as follows:

The maximum average classification accuracy while utilizing variance feature for 2nd stage classification is 80.56%. Among the five kernels used for MCs/mass image classification, linear kernel achieves maximum

classification accuracy while using 4th level variance features of DTMBWT. Maximum average classification accuracy by, quadratic, polynomial, RBF and MLP kernel is 64.13%, 57.87%, 59.34% and 61.03% respectively. It is noted from the Figure 4 that the polynomial and RBF kernel achieves less than 60% classification accuracy.

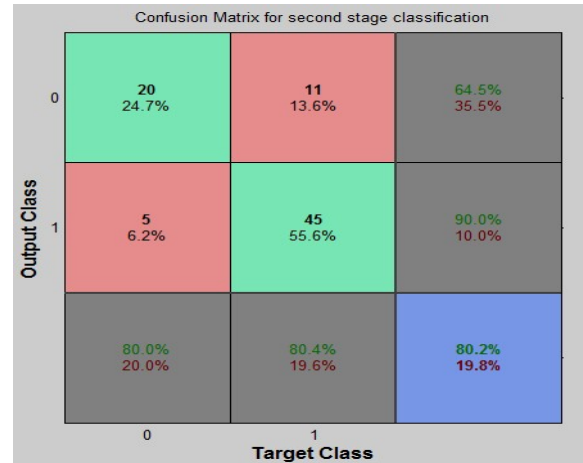

(a) Confusion matrix

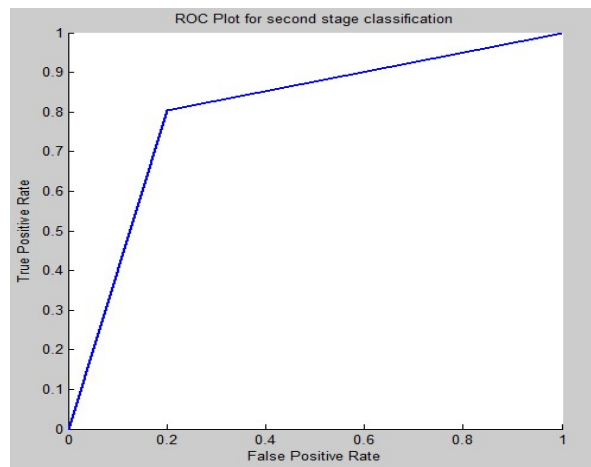

(b) ROC plot

Figure 4: Performance of 2nd stage Classification using DTMBWT Variance Features with Linear Kernel Confusion Matrix and ROC plot

In order to visualize the performance of the proposed 2nd stage classification using DTMBWT variance features and SVM classifier, confusion matrices and ROC plot are shown in Figure 4. It is observed from the Figure 4 that the sensitivity of the proposed system is 80.0% with a specificity of 80.4%. Figure 5 shows overall analysis of classification analysis of evaluated system in stage 2.

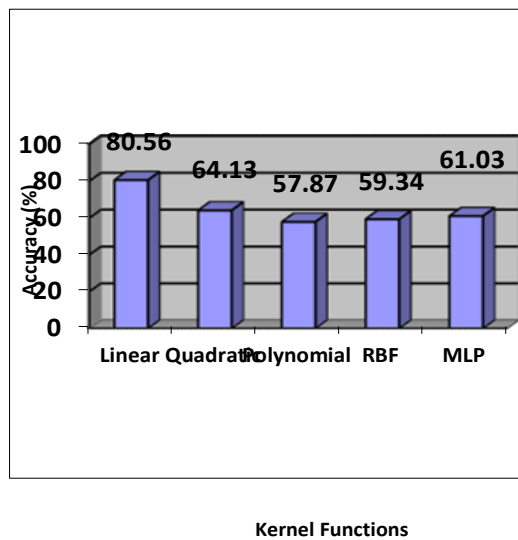


Figure 5: Classification Accuracy vs. SVM Kernels for 2nd Stage Classification using DTMBWT Variance Features

5.3 Third Stage Classification System

The evaluated results of 3rd stage classification system using DTMBWT variance features are illustrated in this section. Table 4 shows the classification accuracy of MCs severity classification.

Table 4: Classification Accuracy for MCs Severity based on DTMBWT Variance Features and SVM Classifier


Level	Over all Classification Accuracy		
	Benign	Malignant	Average
Polynomial			
1	38.67	69.71	54.19
2	73.33	41.86	57.60
3	88.50	64.38	76.44
4	94.33	78.90	86.62
5	92.17	51.21	71.69
6	83.33	45.52	64.43

The interpretations of Table 3 are as follows:


The maximum average classification accuracy while utilizing variance feature is 86.62% for the classification of MCs into benign/malignant. Among the five kernels used for MCs benign and malignant image classification, polynomial kernel achieves maximum classification accuracy while using 4th level variance features of DTMBWT. Maximum average classification accuracy by

linear, quadratic, RBF and MLP kernel is 70.77%, 69.15%, 67.26% and 62.98% respectively.

In order to visualize the performance of the proposed 3rd stage MCs classification using DTMBWT variance features and SVM classifier, confusion matrices and ROC plot are shown in Figure 6. It is observed from the Figures 6 that the 0.840 AUC is achieved while using polynomial kernel. It is observed from the Figure 6 that the sensitivity of the proposed system is 76.9% with a specificity of 91.7%. Figure 5 shows overall analysis of classification analysis of evaluated system in stage 3 MCs Classification.

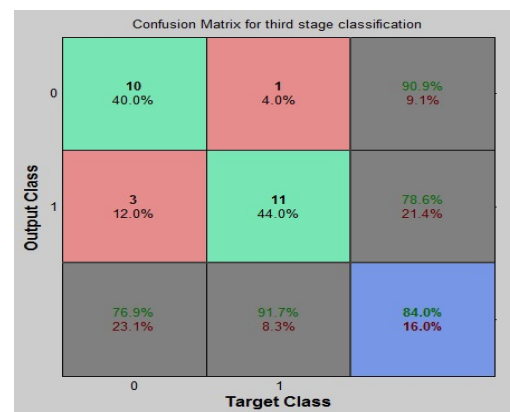

(a) Confusion Matrix

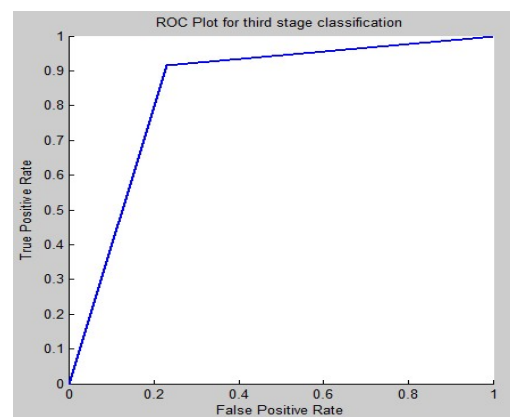

(b) ROC plot

Figure 6: Performance of 3rd Stage MCs Classification using DTMBWT Variance Features with Polynomial Kernel

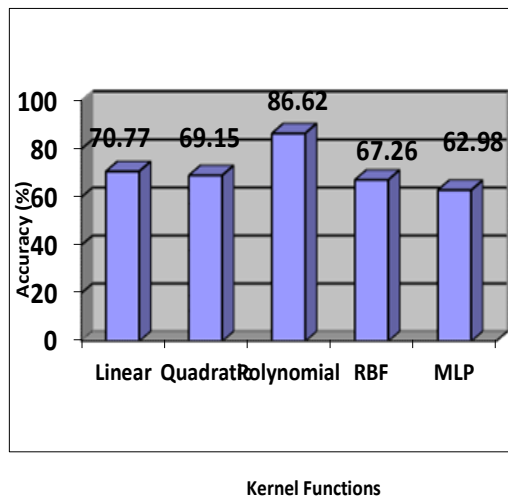


Figure 7: Classification Accuracy Vs. SVM Kernels for 3rd Stage MCs Classification using DTMBWT Variance Features

The evaluated results of 3rd stage classification system using DTMBWT variance features are illustrated in this section. Table 5 shows the classification accuracy of Mass severity classification.


Table 5: Classification Accuracy for Mass Severity Based on DTMBWT Variance Features and SVM Classifier

Level	Overall Classification Accuracy		
	Benign	Malignant	Average
MLP			
1	24.08	85.65	54.87
2	46.77	74.35	60.56
3	66.73	100.00	83.37
4	55.83	88.65	72.24
5	58.61	69.63	64.12
6	55.61	71.77	63.69


The interpretations of results of Table 5 are as follows: The maximum average classification accuracy while utilizing variance feature is 83.37%. Among the five kernels used for mass severity classification, MLP kernel achieves maximum classification accuracy while using 3rd level variance features of DTMBWT. Maximum average classification accuracy by linear, quadratic, polynomial and RBF kernel is 59.96%, 61.58%, 62.26%, 63.03%

respectively. It is also observed that the quadratic kernel classifies the mass malignant images with 95.00% accuracy while MLP kernel classifies with 100% accuracy.

In order to visualize the performance of the proposed 3rd stage mass classification using DTMBWT variance features and SVM classifier, confusion matrices and ROC plot are shown in Figure 8.

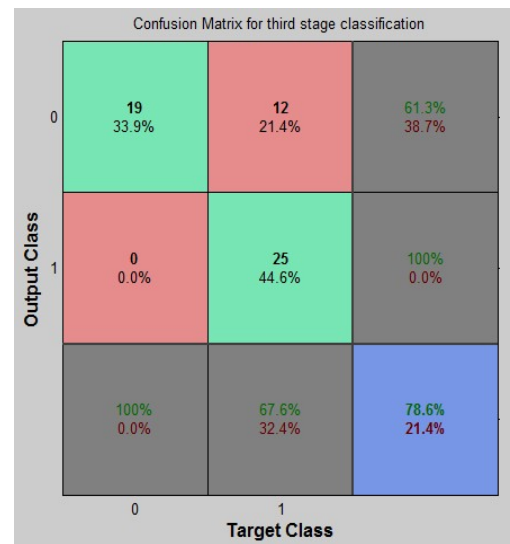

(a) Confusion matrix

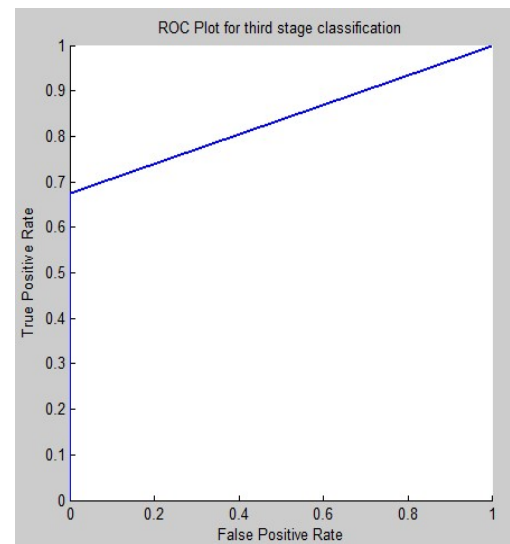

(b) ROC plot

Figure 8: Performance of 3rd Stage Mass Classification using DTMBWT Variance Features with MLP Kernel

It is observed from the Figure 8 that the 0.786 AUC is achieved while using MLP kernel with the sensitivity of the proposed system is 100% with a specificity of 67.6%. Figure 9 shows overall analysis of classification analysis of evaluated system in stage 3 Mass Classification.

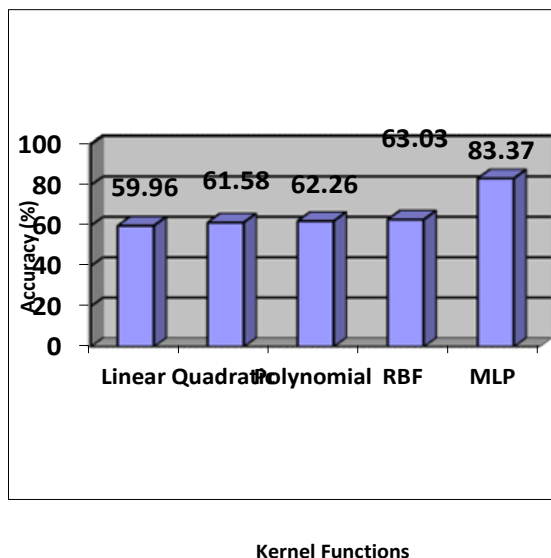


Figure 9: Classification Accuracy Vs. SVM Kernels for 3rd Stage Mass Classification using DTMBWT Variance Features

6. Conclusion

The method employed in this paper has given better performance. The CAD system is developed for the classification of mammogram into 3 stages; Normal/Abnormal Classification in Stage 1, Mass/Micro calcifications (MCs) Classification in Stage 2, Benign/Malignant in Stage 3. This paper has investigated a classification of mammogram images using DTMBWT features. The maximum average classification accuracy rate is 83.50% for normal/ abnormal classification. Classification accuracy for Mass/MCs classification system in 2nd stage 80.56%, Classification accuracy for Mass Severity in 3rd stage 83.37%. For future work, GLCM features combined with statistical moment features to improve statistical properties of DTMBWT coefficients, other textural features can be used to improve the results in the classification of digital mammogram images. For future work, Hybrid classifier or ensemble based classification can be used for further improvement.

References

- [1] www.breastcancer.org
- [2] Brijesh Verma and Ping Zhang."A novel neural-genetic algorithm to find the most significant combination of features in digital mammograms", Applied Soft Computing, no.7, pp.513-525, 2007.
- [3] Marrocco, C., M. Molinara, C. D'Elia and F. Tortorella,2010. "A Computer Aided Detection System for Clustered microcalcifications. Artif. Intell. Med., 50:23-32. DOI: 10.1016/j.artmed.2010.04.007.
- [4] R. Nithya and B. Santhi." Classification of Normal and Abnormal Patterns in Digital Mammograms for Diagnosis of Breast Cancer, International Journal of Computer Applications (0975 – 8887), Volume 28– No.6, August 2011.
- [5] Aidarus M. Ibrahim, Baharum Baharudin, Abas Md Said and P.N. Hashimah," Classification of Breast Tumor in Mammogram Images Using Unsupervised Feature Learning", Science Publications, Original Research Paper,2016.
- [6] Mini MIAS Database Information available at: <http://mammoimage.org/database>.
- [7] Caroline Chaux , Laurent Duva and Jean-Christophe Pesquet. "2D Dual-Tree M-Band Wavelet Decomposition".
- [8] Selesnick.I.W."The Double-Density Dual-Tree DWT", IEEE Transaction on Signal Processing, 52(5), 1304-1314, 2004.
- [9] Cheng. H. D. & Cui. M. (2004). "Mass Lesion Detection with a Fuzzy Neural Network's", 37(6), 1189-1200.
- [10] Verma. B., McLeod. P, & Klevansky. A. (2010). "Classification of Benign and Malignant Patterns in Digital Mammograms for the Diagnosis of Breast Cancer".Expert Systems with Applications, 37(4), 3344-3351.